

INTERNATIONAL
STANDARD

ISO
10893-7

Second edition
2019-02

**Non-destructive testing of steel
tubes —**

**Part 7:
Digital radiographic testing of the
weld seam of welded steel tubes for
the detection of imperfections**

Essais non destructifs des tubes en acier —

*Partie 7: Contrôle par radiographie numérique du cordon de soudure
des tubes en acier soudés pour la détection des imperfections*

STANDARDSISO.COM : Click to View the full PDF of ISO 10893-7:2019



Reference number
ISO 10893-7:2019(E)

© ISO 2019

STANDARDSISO.COM : Click to view the full PDF of ISO 10893-7:2019



COPYRIGHT PROTECTED DOCUMENT

© ISO 2019

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Fax: +41 22 749 09 47
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

	Page
Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 General requirements	3
5 Test equipment	3
6 Test method	4
7 Image quality	6
8 Image processing	11
9 Classification of indications	12
10 Acceptance limits	12
11 Acceptance	13
12 Image storage and display	13
13 Test report	13
Annex A (informative) Examples of distribution of imperfections	15
Bibliography	17

STANDARDSISO.COM : Click to view the full PDF of ISO 10893-7:2019

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 17, *Steel*, Subcommittee SC 19, *Technical delivery conditions for steel tubes for pressure purposes*.

This second edition cancels and replaces the first edition (ISO 10893-7:2011), which has been technically revised. The main changes compared with the previous edition are as follows:

- a) some terms and definitions from ISO 17636-2 have been included;
- b) a safety warning for X and gamma rays has been added at the end of [Clause 4](#);
- c) [Figure 2](#) has been aligned with ISO 17636-1 up to 1 000 kV;
- d) the symbols for mathematical formula have been changed in accordance with the ISO/IEC Directives;
- e) it has been clarified in [4.7](#) when the detector size is smaller than the applicable weld length;
- f) “contact technique” has been deleted from the test method in [Clause 6](#);
- g) a reference to ISO 17636-2 has been added in [6.8](#) for additional details related to spatial resolution;
- h) the requirements for duplex wire IQI position have been added in [Clause 7](#);
- i) a reference to ISO 17636-2 for the calibration of DDAs has been added in [Clause 8](#);
- jj) [Figure 4](#) and the figures in [Annex A](#) have been revised.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Introduction

Digital radiography has been used for the testing of longitudinal weld seams in submerged arc-welded steel tubes for some years. Digital radiography can be automated, and is considered to be more environmentally friendly than film-based radiographic techniques.

Digital radiography maintains the levels of security and availability afforded by X-ray film testing, which have been in place for many years. Images can be made available in a fraction of the time previously taken by film-based techniques, and usually at a lower exposure level and increased detector unsharpness when compared to film.

The storage and handling of digital images maintain the same levels of integrity available from film-based techniques, yet gain all the benefits associated with comprehensive data storage and retrieval systems.

Imaging systems are constantly under development, and an important aspect of this document is to qualify the use of those alternative systems currently available. This document describes the steps required to deliver these benefits.

STANDARDSISO.COM : Click to view the full PDF of ISO 10893-7:2019

Non-destructive testing of steel tubes —

Part 7:

Digital radiographic testing of the weld seam of welded steel tubes for the detection of imperfections

1 Scope

This document specifies the requirements for digital radiographic X-ray testing by either computed radiography (CR) or radiography with digital detector arrays (DDAs) of the longitudinal or helical weld seams of automatic fusion arc-welded steel tubes for the detection of imperfections. This document specifies acceptance levels and calibration procedures.

It can also be applicable to the testing of circular hollow sections.

NOTE As an alternative, see ISO 10893-6 for film-based radiographic X-ray testing.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 5576, *Non-destructive testing — Industrial X-ray and gamma-ray radiology — Vocabulary*

ISO 9712, *Non-destructive testing — Qualification and certification of NDT personnel*

ISO 11484, *Steel products — Employer's qualification system for non-destructive testing (NDT) personnel*

ISO 17636-2:2013, *Non-destructive testing of welds — Radiographic testing — Part 2: X- and gamma-ray techniques with digital detectors*

ISO 19232-1, *Non-destructive testing — Image quality of radiographs — Part 1: Determination of the image quality value using wire-type image quality indicators*

ISO 19232-2, *Non-destructive testing — Image quality of radiographs — Part 2: Determination of the image quality value using step/hole-type image quality indicators*

ISO 19232-5, *Non-destructive testing — Image quality of radiographs — Part 5: Determination of the image unsharpness and basic spatial resolution value using duplex wire-type image quality indicators*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 5576, ISO 11484 and the following apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>

3.1

tube

hollow long product open at both ends, of any cross-sectional shape

3.2

welded tube

tube (3.1) made by forming a hollow profile from a flat product and welding adjacent edges together, and which after welding can be further processed, either hot or cold, into its final dimensions

3.3

manufacturer

organization that manufactures products in accordance with the relevant standard(s) and declares the conformity of the delivered products with all applicable provisions of the relevant standard(s)

3.4

agreement

contractual arrangement between the *manufacturer* (3.3) and the purchaser at the time of enquiry and order

3.5

signal-to-noise ratio

SNR

S/N

ratio of mean value of the linearized grey values to the standard deviation of the linearized grey values (noise) in a given region of interest in a digital image

[SOURCE: ISO 17636-2:2013, 3.10, modified — The symbol *S/N* has been added.]

3.6

basic spatial resolution of a digital detector

$R_{bs_{\text{detector}}}$

resolution that corresponds to half of measured detector unsharpness in a digital image and to the effective pixel size, and indicates the smallest geometrical detail, which can be resolved with a digital detector at a magnification equal to one

Note 1 to entry: For this measurement, the duplex wire image quality indicator (IQI) is placed directly on the digital detector array or imaging plate.

Note 2 to entry: The measurement of unsharpness is described in ISO 19232-5, see also ASTM E2736 and ASTM E1000.

[SOURCE: ISO 17636-2:2013, 3.8, modified — The symbol has been changed from SR_b_{detector} .]

3.7

representative quality indicator

RQI

real part, or a fabrication of similar geometry in radiologically similar material to a real part, that has features of known characteristics that represent those features of interest for which the parts to be purchased are being examined

[SOURCE: ASTM E1817:2008]

3.8

digital detector array system

DDA system

electronic device converting ionizing or penetrating radiation into a discrete array of analogue signals, which are subsequently digitized and transferred to a computer for display as a digital image corresponding to the radiologic energy pattern imparted upon the input region of the device

[SOURCE: ISO 17636-2:2013, 3.3]

4 General requirements

4.1 Unless otherwise specified by the product standard or agreed on by the manufacturer and the purchaser, a radiographic inspection shall be carried out on welded tubes after completion of all the primary manufacturing process operations (rolling, heat treating, cold and hot working, sizing and primary straightening, etc.).

4.2 This inspection shall be carried out by trained operators who are certified (e.g. ISO 9712) or qualified (e.g. ISO 11484 or ASNT SNT-TC-1A), and supervised by competent personnel nominated by the manufacturer. In the case of third-party inspection, this shall be agreed on between the manufacturer and the purchaser.

The operating authorization issued by the employer shall be according to a written procedure. Non-destructive testing (NDT) operations shall be authorized by a level 3 NDT individual approved by the employer.

NOTE The definitions of levels 1, 2 and 3 can be found in the appropriate standards, e.g. ISO 9712 and ISO 11484.

4.3 The tubes under test shall be sufficiently straight and free of foreign matter as to ensure the validity of the test. The surfaces of the weld seam and adjacent parent metal shall be sufficiently free of such foreign matter and surface irregularities, which would interfere with the interpretation of the radiographs.

Surface grinding is permitted in order to achieve an acceptable surface finish.

4.4 In cases where the weld reinforcement is removed, markers, usually in the form of lead arrows, shall be placed on each side of the weld such that its position can be identified on the radiographic image. Alternatively, an integrated automatic positioning system may be used to identify the position of the weld.

4.5 Identification symbols, usually in the form of lead letters, shall be placed on each section of the weld seam radiograph such that the projection of these symbols appears in each radiographic image to ensure unequivocal identification of the section. Alternatively, an integrated automatic positioning system may be used to identify the position of each radiographic image along the pipe weld.

4.6 Markings shall be displayed on the recorded radiographic images to provide reference points for the accurate relocation of the position of each radiograph. Alternatively, the automated measured image position may be displayed on the digital image viewing screen by software for accurate position relocation.

4.7 When the detector size is smaller than the applicable weld length, the pipe or the detector shall move into start-stop mode and digital radiographs shall be taken when the pipe is not moving.

WARNING — Exposure of any part of the human body to X-rays or gamma-rays can be highly injurious to health. Wherever X-ray equipment or radioactive sources are in use, appropriate safety measures shall be applied.

Local, national or international safety precautions when using ionizing radiation shall be strictly applied.

5 Test equipment

The following digital imaging methods can be used in replacement of radiographic film:

- CR with storage phosphor imaging plates (e.g. EN 14784-1 and EN 14784-2);
- radiology with DDAs (e.g. ASTM E2597-07 and ASTM E2698);

c) digital radioscopy with image integration (e.g. EN 13068-1, EN 13068-2 and EN 13068-3).

6 Test method

6.1 The weld seam shall be tested by a digital radiographic technique, corresponding to [Clause 5](#) a) to c).

6.2 Two image quality classes, A and B, conforming to ISO 17636-2, shall be specified:

- class A: radiographic examination technique with standard sensitivity;
- class B: radiographic technique with enhanced sensitivity.

NOTE Image quality class A is used for most applications. Image quality class B is intended for applications where increased sensitivity is required to reveal all the imperfections being detected.

The required image quality class should be stated in the relevant product standard.

6.3 The digital image displayed shall meet the required image quality class A or B.

6.4 The beam of radiation shall be directed at the centre of the section of the weld seam under examination and shall be normal to the tube surface at that point.

6.5 The diagnostic length shall be such that the increase in penetrated thickness at the ends of the useful length of the sensitive detector input screen shall not exceed the penetrated thickness at the centre of the detector by more than 10 % for image quality class B or by more than 20 % for image quality class A, provided the specific requirements of [6.9](#) and [Clause 7](#) are satisfied.

6.6 The single wall penetration technique shall be used. When the single wall technique is impracticable for dimensional reasons, the use of the double wall penetration technique may be used, by agreement, if the required sensitivities can be shown to be achievable.

6.7 If the geometric magnification technique (see [6.8](#)) is not used, the detector shall be placed as close to the object as possible.

The minimum value of the source-to-weld distance, f , shall be selected such that the ratio of this distance to the effective focal spot size, d , i.e. f/d , conforms to the values given by [Formulae \(1\)](#) and [\(2\)](#):

for image quality class A:

$$\frac{f}{d} \geq 7,5 \times b^{\frac{2}{3}} \quad (1)$$

for image quality class B:

$$\frac{f}{d} \geq 15 \times b^{\frac{2}{3}} \quad (2)$$

where b is the distance between the source side of the weld and the sensitive surface of the detector, in millimetres.

NOTE These relationships are presented graphically in [Figure 1](#).

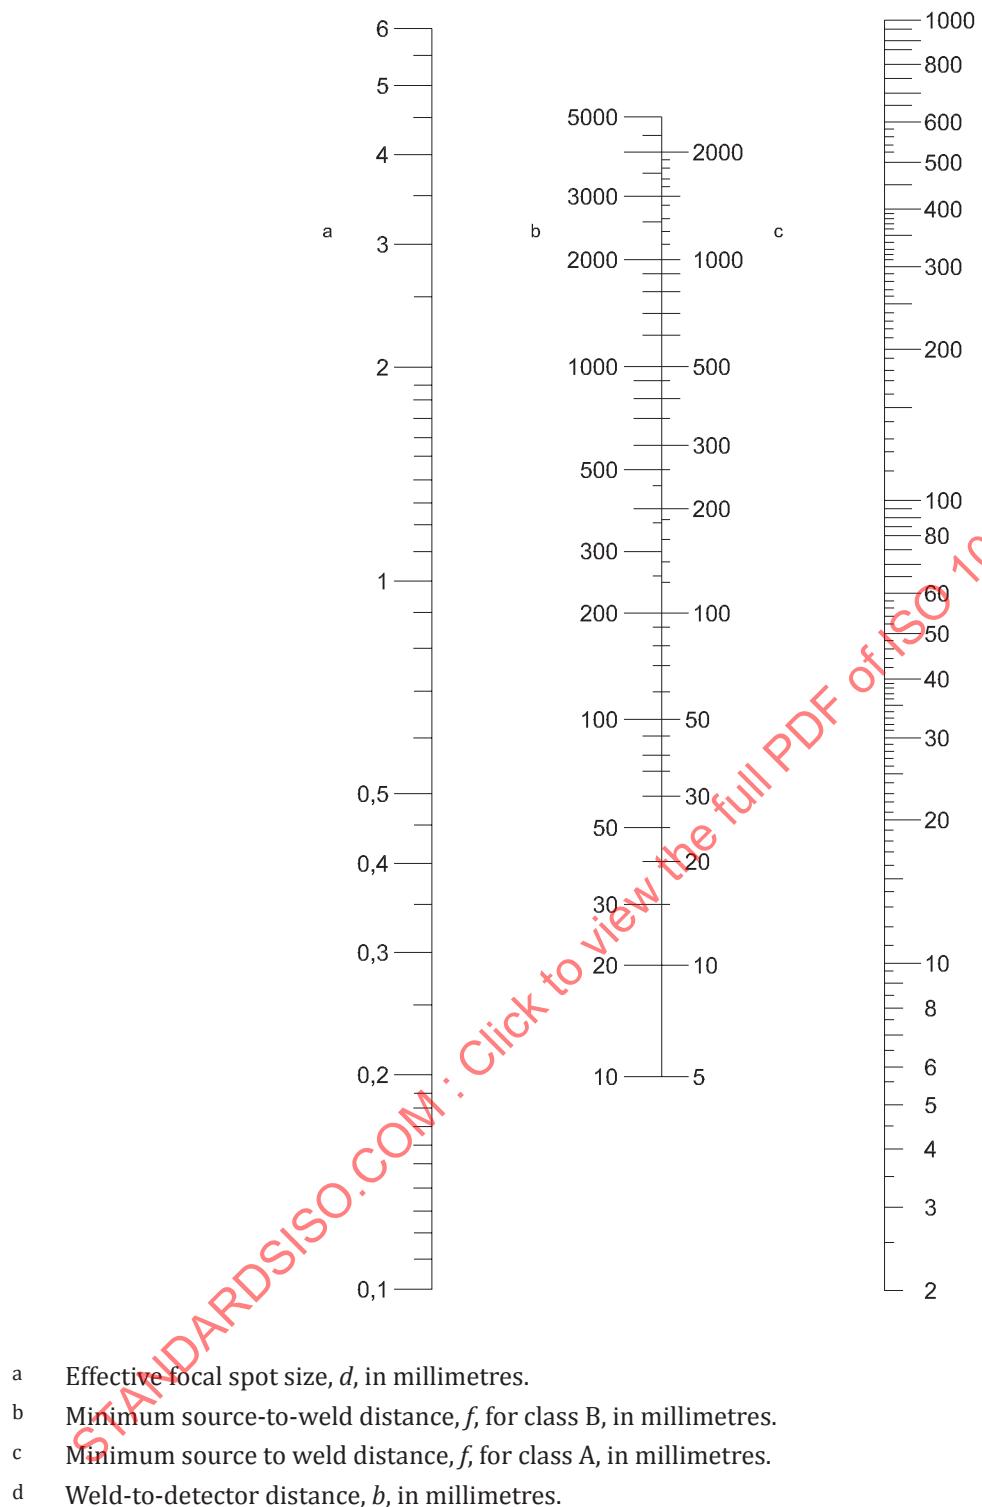


Figure 1 — Nomogram for determination of minimum source-to-weld distance, f , in relation to weld-to-detector distance, b , and the effective focal spot size, d

6.8 An obstacle to the implementation of DDA systems is the large ($> 50 \mu\text{m}$) pixel size of the array compared to the small grain size in film (which leads to film having very high spatial resolution).

It can, therefore, not be possible to achieve the required geometric resolution with a setup typically used for film radiography. This difficulty may be circumvented by using geometric magnification to achieve the required geometric resolution or by making use of the compensation principle [increasing


the signal-to-noise ratio (SNR) in the image] described in 7.1. Any combination of these measures is allowed.

For additional details related to spatial resolution, refer to ISO 17636-2:2013, 7.7.

6.9 Exposure conditions, including X-ray tube voltage, shall achieve the image quality indicator (IQI) requirements in Clause 7. Image contrast and brightness may be adjusted as required for digital image viewing.

6.10 To maintain good flaw sensitivity, the X-ray tube voltage should be as low as possible and the S/N_N in the digital image should be as high as possible. Recommended maximum values of X-ray tube voltage versus penetrated thickness are given in Figure 2. These maximum values are best practice values for film radiography.

After accurate calibration, DDAs can provide sufficient image quality at significantly higher voltages than those shown in Figure 2.

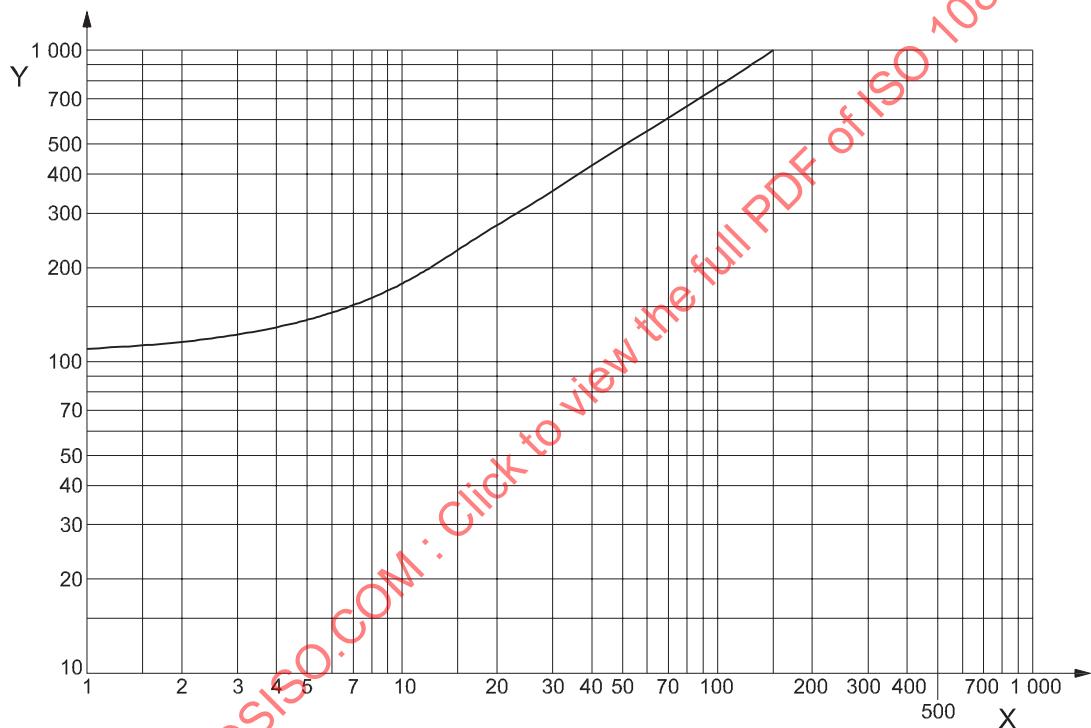

Key

X penetrated thickness, in mm


Y X-ray voltage, in kV

Figure 2 — Maximum X-ray voltage for X-ray devices up to 1 000 kV as a function of penetrated thickness

7 Image quality

7.1 The image quality shall be determined by the use of IQIs of the type specified in ISO 19232-1, ISO 19232-2 and ISO 19232-5, and agreed on between the manufacturer and the purchaser. The


appropriate IQI shall be placed on the source side of the weld on the base material adjacent to the weld. (see [Figures 3 and 4](#)).

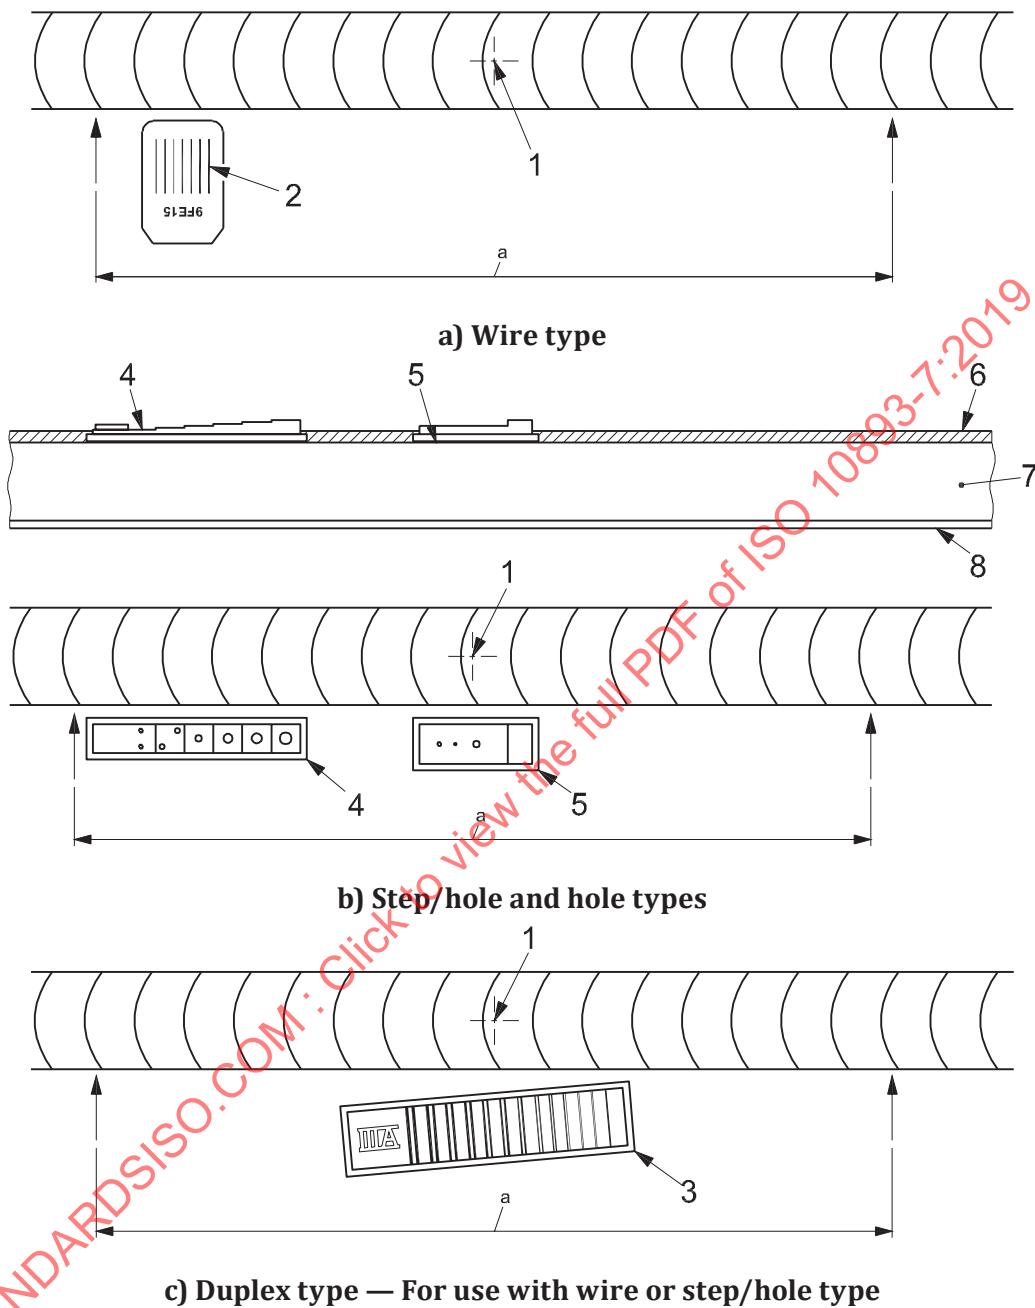

Key

- 1 centre of beam
- 2 wire type IQI, thinnest wire away from the centre of the beam
- 3 duplex type IQI, approx. 5° tilted
- 4 step/hole type IQI, thinnest step away from the centre of the beam
- 5 hole type IQI, if necessary with shim stock
- 6 outer weld reinforcement
- 7 tube wall
- 8 inner weld reinforcement
- a Mapped weld length (DDA) or image plate length (CR).

Figure 3 — Positioning of IQIs — Basic requirements

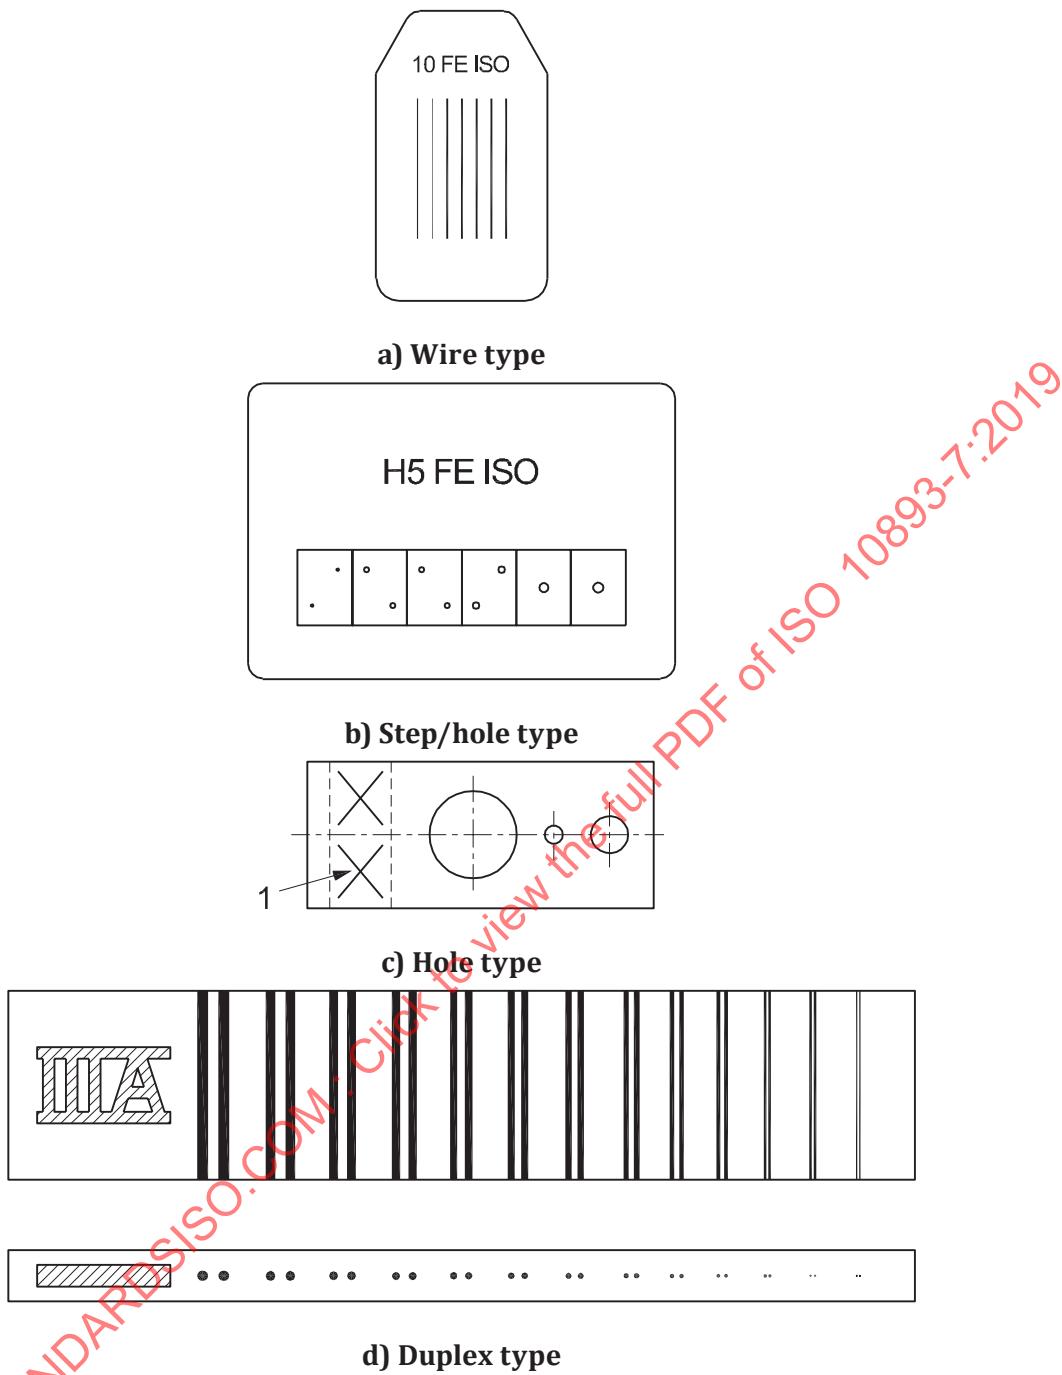**Key**

1 place identification number here

NOTE [Figure 4 c\)](#) is a hole-type IQI of ASTM E1025.

Figure 4 — Types of image quality indicator

When using a wire IQI, the wires shall be directed perpendicular to the weld and its location shall ensure that at least 10 mm of the wire length shows in a section of the metal adjacent to the weld. If requested, an additional or longer IQI shall be placed across the weld.

When the source side is inaccessible, the IQIs may be placed on the detector side of the object. In these circumstances, a letter "F" shall be placed near the IQIs and this procedural change shall be recorded in the test report.

Detector-side positions typically show 1 or 2 more wires, or holes, than if the same IQI was on the source side. Customers may ask for a trial exposure to be carried out on a sample piece of pipe, with IQIs placed on both source and detector sides as a comparison, see ISO 17636-2:2013, 6.7, for details

When the tubes under inspection have the same dimensions and grade, it is sufficient to use the IQI only every 4 h, or twice a shift, to check image sensitivity. When carrying out the sensitivity checks, though, the IQI shall be placed on the source side.

The parameters used with the trial exposures (settings of X-ray source, detector and geometry) shall not be changed for the subsequent images acquired with detector-side IQIs. For stable systems and processes, such as automated testing systems using DDAs, it is sufficient to prove the image quality once per shift as long as the tube dimension, tube material and testing parameters remain unchanged. In this case, the image quality proof should be performed only with source side IQIs.

By usage of the duplex wire IQI, conforming to ISO 19232-5, the image unsharpness, U_g , shall be measured.

The read-out unsharpness, U_g , value for the duplex wire IQI is the smallest wire pair element number (largest wire diameter) with a dip separation below 20 %, measured with a profile plot across the duplex wire in the digital image.

The duplex wire IQI should be positioned on the surface of parent metal at an approximately 5° angle towards the pixel orientation in order to avoid aliasing effects.

7.2 The basic spatial resolution of the digital detector, R_{bs}^{detector} , which is fixed by the construction and hardware parameters, shall be determined by placing the duplex wire IQI directly in front of the detector. In this case, R_{bs}^{detector} , is given by [Formula \(3\)](#).

$$R_{bs}^{\text{detector}} = 0,5 U_g \quad (3)$$

Compensation principle: if both IQI sensitivities of [Tables 1](#) and [2](#) (wire or hole and duplex wire IQI) cannot be achieved by the detector system used, an increase in single wire visibility can compensate too high unsharpness values. This compensation shall be limited to max 3 IQI values.

EXAMPLE For 10 mm wall thickness, class B; it is necessary to use wire number W14 and duplex D11. If D11 cannot be reached, compensation is possible: two steps down from D11 to D9, but increasing two steps up from W14 to W16.

The contrast sensitivity for digital detectors depends on the integration time and tube current (mA) used for the acquisition of the radiographic images for a given distance and tube voltage, so the single wire visibility can be increased by an increased exposure time and mA setting.

7.3 The two image quality classes are defined in [Tables 1](#) and [2](#). The minimum normalized S/N_{norm} in the base material should be > 70 for testing class A and > 100 for testing class B. The normalized S/N_{norm} shall be calculated from the measured S/N in the image at base material adjacent to the welding seam and normalized by the basic spatial resolution of the detector system:

$$S/N_{\text{norm}} = S/N \times 88,6 \mu\text{m} / R_{bs}^{\text{detector}} \quad (4)$$

NOTE For details of SNR measurement, see, for example, EN 14784-1, ASTM E2446-05 or ASTM E2597-07. IQI quality for larger wall thicknesses is available in ISO 17636-2.

7.4 For the double wall penetration technique, the image quality value for use shall be taken as that corresponding to twice the specified wall thickness.

7.5 Where available, the performance of the digital system should also be measured, using representative quality indicators (RQIs). RQIs should be of the same dimensions and radiographic

absorption characteristics as the tubes under inspection. RQIs use are advised in order to ensure digital set-up is capable of meeting inspection specifications.

7.6 The two image quality classes are defined in [Tables 1](#) and [2](#).

Table 1 — Single wall techniques — Class A

Dimensions in millimetres

Specified wall thickness <i>T</i>	Wire number Diameter	Specified wall thickness <i>T</i>	Hole number Diameter	Specified wall thickness <i>T</i>	Duplex IQI ^{a,b} Unsharpness	Wire diameter ^c and spacing
$T \leq 1,2$	W18 0,063	$T \leq 2$	H3 0,20	$T \leq 2$	D11 0,16	0,080
$1,2 < T \leq 2$	W17 0,08	$2 < T \leq 3,5$	H4 0,25	$2 < T \leq 5$	D10 0,20	0,100
$2 < T \leq 3,5$	W16 0,10	$3,5 < T \leq 6$	H5 0,32	$5 < T \leq 10$	D9 0,26	0,130
$3,5 < T \leq 5$	W15 0,13	$6 < T \leq 10$	H6 0,40	$10 < T \leq 25$	D8 0,32	0,160
$5 < T \leq 7$	W14 0,16	$10 < T \leq 15$	H7 0,50	$25 < T \leq 55$	D7 0,40	0,200
$7 < T \leq 10$	W13 0,20	$15 < T \leq 24$	H8 0,64	$55 < T$	D6 0,50	0,250
$10 < T \leq 15$	W12 0,25	$24 < T \leq 30$	H9 0,80			
$15 < T \leq 25$	W11 0,32	$30 < T \leq 40$	H10 1,00			
$25 < T \leq 32$	W10 0,40	$40 < T \leq 60$	H11 1,25			
$32 < T \leq 40$	W9 0,50	$60 < T$	H12 1,60			
$40 < T \leq 55$	W8 0,63					
$55 < T$	W7 0,80					

^a Duplex IQI should be used in conjunction with either a wire or step/hole IQI.

^b Duplex IQI should be examined using a profile display; the smallest wires which have a dip separation below 20 % between the wire pair determine the unsharpness.

^c Basic spatial resolution as determined with a duplex wire IQI on the source side of the object in accordance with ISO 17636-2:2013, Annex C.

Table 2 — Single wall techniques — Class B

Dimensions in millimetres

Specified wall thickness <i>T</i>	Wire number Diameter	Specified wall thickness <i>T</i>	Hole number Diameter	Specified wall thickness <i>T</i>	Duplex IQI ^{a,b} Unsharpness	Wire diameter ^c and spacing
$T \leq 1,5$	W19 0,05	$T \leq 2,5$	H2 0,16	$T \leq 1,5$	D13+ < 0,10	< 0,05
$1,5 < T \leq 2,5$	W18 0,063	$2,5 < T \leq 4$	H3 0,20	$1,5 < T \leq 4$	D13 0,10	0,05
$2,5 < T \leq 4$	W17 0,08	$4 < T \leq 8$	H4 0,25	$4 < T \leq 8$	D12 0,13	0,065
$4 < T \leq 6$	W16 0,10	$8 < T \leq 12$	H5 0,32	$8 < T \leq 12$	D11 0,16	0,080
$6 < T \leq 8$	W15 0,13	$12 < T \leq 20$	H6 0,40	$12 < T \leq 40$	D10 0,20	0,100
$8 < T \leq 12$	W14 0,16	$20 < T \leq 30$	H7 0,50	$40 < T$	D9 0,26	0,130
$12 < T \leq 20$	W13 0,20	$30 < T \leq 40$	H8 0,64			
$20 < T \leq 30$	W12 0,25	$40 < T \leq 60$	H9 0,80			
$30 < T \leq 35$	W11 0,32	$60 < T$	H10 1,00			
$35 < T \leq 45$	W10 0,40					
$45 < T \leq 65$	W9 0,50					
$65 < T$	W8 0,63					

NOTE "D13+" is achieved if the duplex wire pair D13 is resolved with a dip > 20 %.

^a Duplex IQI should be used in conjunction with either a wire or step/hole IQI.

^b Duplex IQI should be examined using a profile display; the smallest wires which have a dip separation below 20 % between the wire pair determine the unsharpness.

^c Basic spatial resolution as determined with a duplex wire IQI on the source side of the object in accordance with ISO 17636-2:2013, Annex C.

8 Image processing

8.1 The digital data of the radiographic detector shall be evaluated proportional to the radiation dose. This shall be the prerequisite for correct measurements of SNR for evaluation of image quality. For optimal image display, contrast and brightness should be interactively adjustable. Optional filter

functions, profile plots and the SNR tool should be integrated into the software for image display and evaluation.

In order to achieve the required SNR, the calibration of DDAs should be performed in accordance with ISO 17636-2.

NOTE The SNR tool is a special software procedure for signal and noise measurement in region of interest of linearized image raw data (see ISO 17636-2).

8.2 Further means of image processing applied on the stored raw data (e.g. high pass filtering for image display) shall be documented, repeatable and agreed on by the manufacturer and the purchaser.

9 Classification of indications

9.1 All indications found on the radiograph shall be classified as weld imperfections or defects, as described in [9.2](#) and [9.3](#).

9.2 Imperfections are discontinuities in the weld seam detectable by the radiographic testing method described in this document. Imperfections with a size and/or population density within the specified acceptance limits are considered to have no practical implications on the intended use of the tubes.

9.3 Defects are imperfections with a size and/or population density greater than the specified acceptance limits. Defects are considered to adversely affect or limit the intended use of the tubes.

10 Acceptance limits

10.1 Acceptance limits are applicable to radiographic examination of the weld seam and specified in [10.2](#) to [10.6](#), unless alternative requirements are specified in the product standards.

10.2 Cracks, incomplete penetration and lack of fusion are not acceptable.

10.3 Individual circular slag inclusions and gas pockets up to 3,0 mm or $T/3$ in diameter (T = specified wall thickness), whichever is the smaller, are acceptable.

The sum of the diameters of all such permitted individual imperfections in any 150 mm or $12T$ of weld length, whichever is the smaller, shall not exceed 6,0 mm or $0,5T$, whichever is the smaller, where the separation between individual inclusions is less than $4T$.

10.4 Individual elongated slag inclusions up to 12,0 mm or T in length, whichever is the smaller, or up to 1,5 mm in width are acceptable.

The accumulated length of such permitted individual imperfections in any 150 mm or $12T$ of weld length, whichever is the smaller, shall not exceed 12,0 mm where the separation between individual inclusions is less than $4T$.

NOTE For information, the criteria specified in [10.3](#) and [10.4](#) are shown diagrammatically in [Annex A](#).

10.5 Individual undercuts of any length having a maximum depth of 0,4 mm and not encroaching on the minimum wall thickness shall be acceptable.

Individual undercuts of a maximum length of $T/2$ having a maximum depth of 0,5 mm and not exceeding 10 % of the specified wall thickness shall be acceptable, provided there are not more than two such undercuts in any 300 mm of the weld length, and all such undercuts are dressed out.

10.6 Undercuts on the inside and outside welds, which are coincident in the longitudinal direction, shall not be acceptable.

11 Acceptance

11.1 Any tubes not showing indications in excess of that permitted by the corresponding acceptance limits shall be deemed to have passed the test.

11.2 Any tubes showing indications in excess of that permitted by the corresponding acceptance limits shall be deemed suspect.

11.3 For suspect tubes one or more of the following actions shall be taken, subject to the requirements of the product standard.

- a) The suspect area shall be removed by dressing. Complete removal of the defect shall be verified by either liquid penetrant or magnetic particle testing, and the dressed area shall be retested by radiography. The remaining wall thickness shall be measured by an appropriate technique to verify conformity with the specified tolerances.
- b) The suspect area shall be repaired by welding carried out to an approved welding procedure. The repaired area shall then be subject to radiographic examination in accordance with the requirements of this document and the product standard.
- c) The suspect area shall be cropped off. The remaining length of the tube shall be measured to verify conformity with the specified tolerances.
- d) The tube shall be rejected.

12 Image storage and display

The original images shall be stored in full resolution as delivered by the detector system. Only image processing connected with the detector calibration [e.g. off-set correction, gain calibration for detector equalization and bad pixel correction (see ASTM E2597-07) to provide artefact-free detector images] shall be applied before storage of these raw data.

The display for image evaluation should fulfil the following minimum requirements:

- a) minimal brightness of 250 cd/m^2 ;
- b) display of minimal 256 shades of grey;
- c) minimum displayable light intensity ratio of 1:250;
- d) display of minimal $1\ 000 \times 1\ 000$ pixels of a size $< 0,30 \text{ mm}$.

The image evaluation shall be carried out in a dimly lit room. The monitor setup shall be verified with a suitable test image.

It is recommended to use ASTM E2699 for digital imaging and communication in non-destructive evaluation (DICONDE) for digital radiographic test methods.

13 Test report

The manufacturer shall record at least the following information. In addition, if specified, the manufacturer shall submit a test report including the following information unless otherwise agreed by contracting parties:

- a) reference to this document, i.e. ISO 10893-7;

- b) statement of conformity;
- c) any deviation, by agreement or otherwise, from the procedures specified;
- d) product designation by steel grade and size;
- e) radiation source, type and effective focal spot size and equipment used, tube voltage and current;
- f) detector and software used for image acquisition and display;
- g) time of exposure per image, date of last detector calibration;
- h) geometrical set-up, magnification and source-to-pipe distance;
- i) types and positions of image quality indicator (IQI);
- j) IQI readings and minimum SNR at base material;
- k) the image quality class achieved;
- l) file name and storage location of raw data acquired;
- m) date of exposure and report;
- n) operator identification (e.g. code, ID, name/surname), qualification/certification (based on scheme ISO 11484, ISO 9712 or equivalent), level and signature.

STANDARDSISO.COM : Click to view the full PDF of ISO 10893-7:2019