



International
Standard

ISO 14880-3

**Optics and photonics — Microlens
arrays —**

**Part 3:
Test methods for optical properties
other than wavefront aberrations**

Optique et photonique — Réseaux de microlentilles —

*Partie 3: Méthodes d'essai pour les propriétés optiques autres que
les aberrations du front d'onde*

**Second edition
2024-11**

STANDARDSISO.COM : Click to view the full PDF of ISO 14880-3:2024



COPYRIGHT PROTECTED DOCUMENT

© ISO 2024

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Substrate test	1
5 Microscope test method	1
5.1 Principle	1
5.2 Measurement arrangement and test equipment	2
5.2.1 General	2
5.2.2 Test system	3
6 Procedure	4
6.1 General	4
6.2 Measurement of effective back or front focal length	4
6.3 Measurement of chromatic aberration	4
6.4 Measurement of the uniformity of the focal spot positions	5
7 Results and uncertainties	5
8 Coupling efficiency, imaging quality	6
9 Test report	6
Annex A (informative) Measurements with wavefront measuring systems	8
Annex B (informative) Confocal measurement of effective back or front focal length of lens array	10
Annex C (informative) Coupling efficiency, imaging quality	12
Annex D (informative) Measurement of the uniformity of the focal spot positions of a microlens array	13
Bibliography	14

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO document should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

ISO draws attention to the possibility that the implementation of this document may involve the use of (a) patent(s). ISO takes no position concerning the evidence, validity or applicability of any claimed patent rights in respect thereof. As of the date of publication of this document, ISO had not received notice of (a) patent(s) which may be required to implement this document. However, implementers are cautioned that this may not represent the latest information, which may be obtained from the patent database available at www.iso.org/patents. ISO shall not be held responsible for identifying any or all such patent rights.

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 172, *Optics and Photonics*, Subcommittee SC 9, *Laser and electro-optical systems*, in collaboration with the European Committee for Standardization (CEN) Technical Committee CEN/TC 123, *Lasers and photonics*, in accordance with the Agreement on technical cooperation between ISO and CEN (Vienna Agreement).

This second edition cancels and replaces the first edition (ISO 14880-3:2006), which has been technically revised.

The main changes are as follows:

- Introduction revised;
- Reference documents and numbering updated.

A list of all parts in the ISO 14880 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Introduction

This document specifies methods of testing optical properties, other than wavefront aberrations, of microlens arrays. Examples of applications for microlens arrays include three-dimensional displays, coupling optics associated with arrayed light sources and photo-detectors, enhanced optics for liquid crystal displays, and optical parallel processor elements^{[12][13][15][16]}.

The testing of microlenses is in principle similar to testing any other lens. The same parameters need to be measured and similar techniques used. However, in many cases the measurement of very small lenses presents practical problems which make it difficult to use the standard equipment that is available for testing normal size lenses^{[15][16]}.

The market in microlens arrays has generated a need for agreement on basic terminology and test methods. Standard terminology and clear definitions are needed not only to promote applications but also to encourage scientists and engineers to exchange ideas and new concepts based on common understanding.

This document contributes to the purpose of the series of ISO 14880 standards which is to improve the compatibility and interchangeability of lens arrays from different suppliers and to enhance development of the technology using microlens arrays.

Characteristic parameters are defined and examples of applications given in ISO 14880-1. It has been completed by a set of three other International Standards, i.e. ISO 14880-2, ISO 14880-3 and ISO 14880-4.

This document describes the measurement of 1) focal length, 2) coupling efficiency, 3) imaging quality and 4) focal spot positions.

The focal length of the microlens is defined more precisely in ISO 14880-1 as effective back (front) focal length.

The measurement of effective back (front) focal length is described in the body of this part of ISO 14880 and the use of an alternative technique, interferometry, is described in [Annex A](#).

Measurement of the focal length of an array of microlenses, using a confocal technique, is described in the main body and [Annex B](#).

Coupling efficiency and imaging quality are discussed in [Annex C](#).

Measurement of the focal spot positions of an array of microlenses in parallel, using the Shack-Hartmann technique, is described in [Annex D](#).

Wavefront aberrations and characteristics other than optical properties are specified in ISO 14880-2 and ISO 14880-4 and ISO/TR 14880-5.

STANDARDSISO.COM : Click to view the full PDF of ISO 14880-3:2024

Optics and photonics — Microlens arrays —

Part 3:

Test methods for optical properties other than wavefront aberrations

1 Scope

This document specifies methods for testing optical properties, other than wavefront aberrations^[1] of microlenses in microlens arrays. It is applicable to microlens arrays with very small lenses formed on one or more surfaces of a common substrate and to graded-index microlenses.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 14880-1, *Optics and photonics — Microlens arrays — Part 1: Vocabulary*

ISO 10110-5, *Optics and photonics — Preparation of drawings for optical elements and systems — Part 5: Surface form tolerances*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 14880-1 apply.

ISO and IEC maintain terminology databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <https://www.electropedia.org/>

4 Substrate test

The optical quality of the substrate contributes to the quality of the focal positions defined by the microlenses and shall be quantified in accordance with ISO 10110-5.

5 Microscope test method

5.1 Principle

The basic principle is to locate, by optical means, the surface of the microlens under test. The effective back (front) focal length is determined by measuring the axial displacement necessary to locate the focal position.

5.2 Measurement arrangement and test equipment

5.2.1 General

The testing of microlenses is similar in principle to testing larger lenses. In many cases however, the measurement of very small lenses presents practical problems which make it difficult to use standard equipment. In general, two optical techniques can be used. One is based on microscopy, the other is based on interferometry^[2].


The first technique uses a microscope to locate, by focusing, the vertex of the microlens. The effective back (front) focal length is deduced from a measurement of the displacement necessary to refocus the microscope on the image of a distant source as shown in [Figure 1](#).

A focusing aid in the microscope such as a split-field focusing graticule enables the featureless vertex of a microlens to be more readily located when viewing with reflected light. For focal length measurements the distant point source may be the end face of an illuminated optical fibre or an illuminated test graticule. Tests may be performed with white light or monochromatic illumination.

The second technique uses wavefront sensing to locate the test surface or the centre of curvature. The location test may be carried out with the help of one of the following devices:

- Fizeau interferometer,
- Twyman-Green interferometer,
- lateral shearing interferometer, or
- Shack-Hartmann device.

These are more fully described in ISO 14880-2 and ISO/TR 14999-1^{[1][2]}. One advantage of interferometry is that for strongly aberrated lenses, the variation in focal length with aperture radius can be readily deduced from the interference patterns. A disadvantage is that tests are restricted to the wavelength of the interferometer light source.

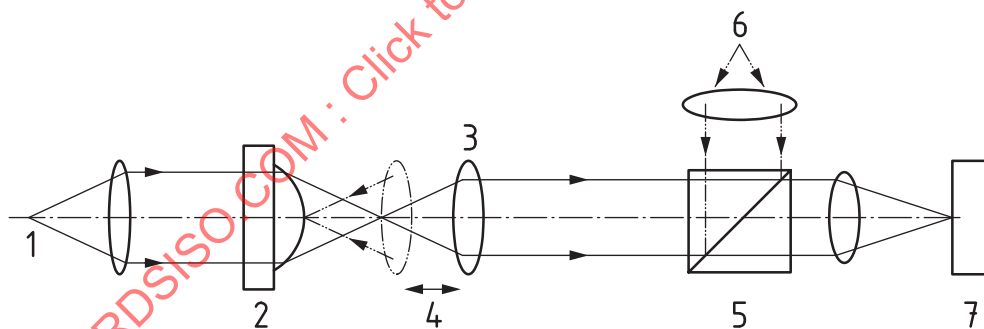

Key

- 1 distant point source
- 2 substrate and microlens producing focused spot
- 3 microscope objective
- 4 axial adjustment of microscope to locate lens surface and focus
- 5 beamsplitter
- 6 source for focus location on lens surface
- 7 imaging array

Figure 1 — Collimated source and microscope used to measure the effective back or front focal length of a microlens

[Clauses 5](#) to [9](#) concentrate on the microscope technique while an interferometric technique is described in [Annex A](#) and a Shack-Hartmann technique in [Annex D](#).

The confocal measurement of the effective focal lengths of lens arrays is described in [Annex B](#).

5.2.2 Test system

5.2.2.1 General

The test system consists of a microscope fitted with displacement transducers, suitable light source, test object, microscope video camera, monitor and image analyser (line intensity scan).

5.2.2.2 Microscope

A microscope fitted with a focusing aid such as a split-image rangefinder is required to enable focus settings to be made on a featureless surface such as the vertex of the microlens surface. The mechanical design shall allow the distant point source or test graticule to be placed below the stage carrying the test lens. Ideally, the test lens should be supported with no additional optical component such as a glass plate between it and the distant point source or test graticule. The displacement of the test surface relative to the microscope objective is measured with a calibrated displacement transducer.

The numerical aperture (NA) of the microscope objective shall be larger than the numerical aperture of the test lens at the focal point.

5.2.2.3 Light source

A light source emitting radiation in the band of wavelengths or at a specific wavelength required for the test shall be used. The properties of the light source shall be described in the test report.

White light can be provided by a quartz-halogen lamp in combination with a suitable aperture stop. Narrow band filters can be used where a restricted range of wavelengths is required. A laser or LED can be used for monochromatic illumination and higher intensities.

5.2.2.4 Test object (test graticule)

The distant point source can be approximated using the end face of an illuminated optical fibre. The distant point source shall be placed on axis with the lens and at an effectively large distance to enable the focal length to be determined.

Alternatively, the object may be a graticule. This enables the optical properties at particular spatial frequencies and field angles to be studied.

The detection of the focus spot may be susceptible to under-sampling by the detector array.

The distant point source or test graticule used shall be described in the documentation of the test report.

5.2.2.5 Image display

If the image generated by the microscope is relayed by a video camera to a video display, an electronic intensity display can be used to assist in locating the position of best focus. The intensity of the image at the detector shall be adjusted to maintain a linear response from the detector system.

5.2.2.6 Standard surfaces

A microlens of known focal length at a defined wavelength shall be used as a calibration artefact to verify the performance of the measurement system.

A step height artefact, for example two thin glass plates held together in optical contact to provide a step of known height, shall be used to verify the performance of the displacement measurement system.

5.2.2.7 Preparation

For consistent results the test equipment shall be maintained in a temperature-controlled environment, preferably at 20 °C and not exposed to vibration.

The optical surfaces to be tested shall be clean. Uncoated glass surfaces may be safely cleaned with alcohol and cotton wool. The cotton wool should be soaked in a very small amount of solvent before touching the surface and wiped only once across the optical surface before being discarded. This minimizes the chances of scratching the surface. Dust may be removed using a clean camel-hair brush or filtered compressed air.

Coated optical surfaces such as antireflection surfaces should be treated with great care and not cleaned unless absolutely necessary. They may be dusted using filtered compressed air.

Guidance should be sought on the correct use of solvents and cleaning materials.

6 Procedure

6.1 General

Clean the surface of the lens and substrate to be tested.

6.2 Measurement of effective back or front focal length

Standard instrument calibration procedures shall be carried out periodically and the calibration uncertainty estimated^{[4][9][10]}.

Verify the performance of the test system by measuring, as described below, the effective back (front) focal length of the standard spherical surface and comparing the result with the known value.

The microscope is focused on the surface of the microlens and then displaced to focus on the image of a graticule or a point source placed at infinity. The best focus position for this image may be located using a camera and display with line scan to determine the displacement position at which the peak intensity in the image is greatest. The spatial resolution of the camera system shall be sufficient to resolve the image. The axial displacement is measured using the displacement transducer.

6.3 Measurement of chromatic aberration

In general, microlenses are of relatively simple design and are not corrected for chromatic aberration. The focal length will vary with wavelength of illumination^[11].

With conventional lenses, a ray is deviated by refraction at the interface between two optical media with distinctly different refractive indices. The magnitude of the paraxial focal length for a single spherical surface of radius R is given by [Formula \(1\)](#):

$$f = R / [n_1(\lambda) - n_2(\lambda)] \quad (1)$$

where n_1 and n_2 are the refractive indices of the two media before and after the interface at a wavelength λ . The chromatic aberration of the lens is determined by the dispersion characteristics of the two media, $n_1(\lambda)$ and $n_2(\lambda)$.

The conventional way of characterizing the dispersion of optical materials is by the Abbe number ν , the definition of which includes values for the refractive index of the material at three wavelengths. For example

480 nm, 546 nm and 644 nm for the Abbe number v_e at the green mercury e-line (546 nm) is given by [Formula \(2\)](#):

$$v_e = (n_{546} - 1) / (n_{480} - n_{644}) \quad (2)$$

The Abbe number usually ranges between 20 and 60. Materials with higher Abbe numbers exhibit less chromatic dispersion than materials with lower Abbe numbers.

The Abbe number of the microlens material may be determined by measuring the focal length of the lens at the appropriate wavelengths and combining [Formulae \(1\)](#) and [\(2\)](#), namely [Formula \(3\)](#):

$$v_{\text{eff}} = (1 / f_{546}) / \left(\frac{1}{f_{480}} - \frac{1}{f_{644}} \right) \quad (3)$$

Various Abbe numbers may be defined depending on the choice of wavelengths. It may be more practical to use laser sources and define the Abbe number at those wavelengths.

The focal length of a lens is measured as described in [6.2](#) using monochromatic illumination. The measurement is then repeated using monochromatic illumination of different wavelengths to derive the chromatic aberration which is defined as [Formula \(4\)](#):

$$\Delta S_z = S_z(\lambda_1) - S_z(\lambda_2) \quad (4)$$

where

$S_z(\lambda)$ is the axial focus position;

λ_1 and λ_2 are the illumination wavelengths with $\lambda_1 > \lambda_2$.

The values obtained relate to the performance of the lens in practice and consideration may have to be given to the dispersion of the substrate.

This method involves measuring small changes of focal length with wavelength and it is important to measure the focal length as accurately as possible to reduce the uncertainty in the value for the Abbe number.

6.4 Measurement of the uniformity of the focal spot positions

Microlens arrays are often used for wavefront measurement such as the Shack-Hartmann test. The lateral shift of the focal spot position from the optical axis represents the angle of the local tilt of the wavefront under test. Therefore reliable data of the uniformity of a microlens array (due to the regular arrangement and the coordinates of the lens aperture centre positions of each individual microlens of the array) are essential for an accurate wavefront measurement.

The disparity of focal spot position shifts of microlenses of an array determines the uniformity of the array.

The test set-up is described in [Annex D](#).

7 Results and uncertainties

The mean value of a set of measured values for focal length should be calculated and recorded. The variance of the set of measured values shall be analysed statistically and the unbiased estimate of the standard deviation evaluated. This is to ascertain the Type A contribution to the expanded uncertainty^[4].

Typical sources of uncertainty are included in [Table 1](#).

Table 1 — Uncertainty considerations

Origin	Type	Uncertainty limit
Focal length measurement	A	Calculated from a set of, typically nine, measurements
Calibration	A/B	Varies with instrument and method of calibration

Optimum measurement conditions can be selected by monitoring the temperature and relative humidity values during the measurements, and always giving the apparatus time to reach room temperature. The Abbe offset error is minimized by arranging for the displacement transducer to measure as close as possible to the optical axis.

8 Coupling efficiency, imaging quality

Microlenses are often used to collimate light from a small source such as a laser diode, to focus light to a small aperture or to couple light into a fibre. In other applications, microlenses are used to generate small images of an object. The coupling efficiency and the imaging quality of microlens arrays are discussed in [Annex C](#).

9 Test report

The test results shall be recorded and shall include the following information if applicable:

- a) General information:
 - 1) test has been performed according to ISO 14880-3:2024;
 - 2) date of calibration, calibration procedure and calibration uncertainty assessment;
 - 3) date of test;
 - 4) name and address of test organization;
 - 5) accreditation (if relevant);
 - 6) name of individual performing the test.
- b) Information about the lens under test:
 - 1) lens type;
 - 2) manufacturer;
 - 3) manufacturer's model;
 - 4) serial number.
- c) Environmental test conditions:
 - 1) temperature;
 - 2) relative humidity.
- d) Information concerning testing and evaluation:
 - 1) test method used;
 - 2) optical system used;
 - 3) light source:
 - i) source type,

- ii) wavelength;
- 4) displacement transducer used.
- e) Test results:
 - 1) effective back focal length;
 - 2) effective front focal length;
 - 3) focal spot position shifts ΔS_x and ΔS_y ;
 - 4) chromatic aberration: ΔS_z ;
 - 5) uncertainty table.

STANDARDSISO.COM : Click to view the full PDF of ISO 14880-3:2024

Annex A (informative)

Measurements with wavefront measuring systems

A.1 Interferometer measurement principle

A variety of methods exist for measuring the focal length of lenses^[5]. Back (front) focal length may be measured using an interferometer to help locate the vertex of the lens surface and to find the best focus position and using a linear displacement transducer for length measurement. One of the following devices could be used for this purpose^[5]:


- Fizeau interferometer;
- Twyman-Green interferometer^[6];
- lateral shearing interferometer, or
- Shack-Hartmann device.

Use of a Fizeau interferometer is described here as an example. A collimated beam from a coherent light source is partially reflected from a plane reference surface to generate a reference wavefront. The transmitted light is focused to a spot by a high quality lens and this spot is used to probe the position of the lens surface and the focal point. Interference patterns are monitored to determine the two locations.

NOTE For strongly aberrated microlenses, the effective focal length as defined in ISO 14880-1 may differ significantly from values based on wavefront deviation criteria.

A.2 Measurement arrangement and test equipment

The Fizeau interferometer is shown in [Figure A.1](#).

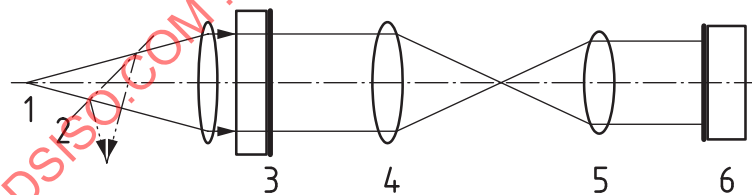

Key

- 1 coherent light source and collimator
- 2 beamsplitter
- 3 reference plane
- 4 high quality microscope objective
- 5 microlens under test
- 6 optical flat

Figure A.1 — Fizeau interferometer

In principle, interferometers available for testing conventional sized lenses, particularly those of the Fizeau type, may appear to be suitable for measurements with microlenses. In practice, problems may arise from stray reflections from secondary surfaces in close proximity to the surface under test. The relatively high magnification involved may lead to difficulties in focusing on the test surfaces of the microlens.

Interferometers specially designed for microsurfaces overcome these problems^[6]. The optical flat is positioned as close as possible to the microlens under test to minimize aperture diffraction errors and focus the lens array onto the detector array.

A.3 Measurement of effective back or front focal length

To measure focal length, the microlens under test is positioned on-axis so as to collimate the diverging beam. A high quality plane mirror or optical flat is used to reflect the light back through the system where it combines with the reference wavefront to form an interference pattern. It is advisable to first align the plane mirror without the microlens and microscope objective in place by tilting the plane mirror until the interference pattern is nulled, that is the intensity is uniformly distributed. The microscope objective and microlens are then inserted and the axial position of the microlens is adjusted until the interference pattern is again nulled. Alternatively, a small tilt may be introduced between the two wavefronts to generate a pattern of interference bands and the setting is made by adjusting the axial position of the microlens until the bands are straight, parallel and equidistant^[9].

The lens under test is then moved axially until the probe beam is focused on the lens surface. In this position, the light is partially reflected in the cat's eye configuration back to the interferometer to form a pattern of bands. The lens position is adjusted until the bands are either nominally straight or nulled.

Focal length measurements are deduced from the axial displacements of the test lens between the positions discussed above. Such measurements may be conveniently made with a laser length measuring interferometer.

NOTE In practice, totally straight interference bands will rarely be obtained. The effect of aberrations in the lens under test will be to introduce bending of the interference bands that will vary over the field. Residual aberrations in the test system can also be apparent especially when using the cat's eye configuration which inverts one wavefront with respect to the other.

Annex B (informative)

Confocal measurement of effective back or front focal length of lens array

B.1 Measurement principle


The effective back (front) focal length of multiple lenses in the array can be measured using the confocal principle with light focused by a single lens as shown in [Figure B.1](#)^[14].

A plane mirror surface in Position A shall be located by focusing light to the surface where it is reflected in the cat's eye configuration. Light reflected back through the lens is reflected at a beam-splitter and focused to a pinhole. Light transmitted by the pinhole is detected electronically.

When the mirror surface is positioned at the focal point of the microlens, the light reflected back through the pinhole is at a maximum. If the distance from the lens to the mirror surface is reduced, a position is found at Position B where the intensity of light transmitted by the pinhole reaches a secondary maximum. In this position, light is reflected from the lens surface in the cat's eye configuration.

The distance between the two positions is one half of the effective focal length of the microlens.

By replacing the lens with a microlens array the mean effective focal length of the array can be measured.

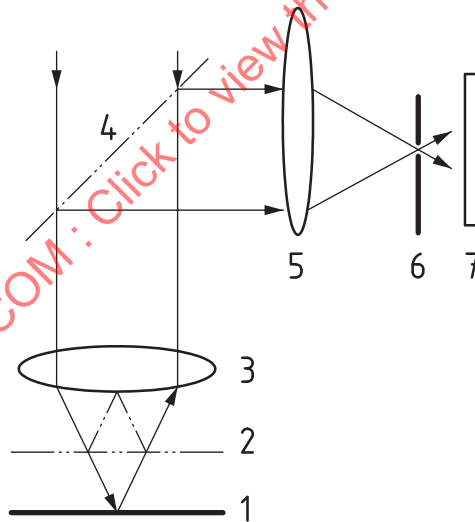


Key

- 1 mirror surface Position A
- 2 mirror surface Position B
- 3 microlens
- 4 beamsplitter
- 5 focusing lens
- 6 pinhole
- 7 detector

Figure B.1 — Measurement of the effective focal length of a microlens array

B.2 Measurement system for microlens arrays

A confocal optical system and a plane mirror on an adjustable stage equipped with a displacement transducer is required as shown in [Figure B.2](#). The mirror is positioned close to the focal plane of the lens array and the axial position adjusted until maximum light is transmitted by the pinhole. The detector array, for example a CCD, enables the spatial distribution of bundles of rays from each microlens aperture to be monitored. The axial position of the mirror is scanned and the position that corresponds to maximum intensity at the CCD for each lens element is recorded.

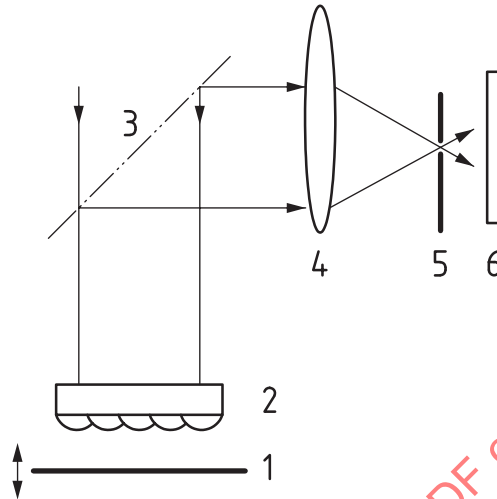

Key

- 1 mirror positioned at microlens array focal plane
- 2 microlens array
- 3 beamsplitter
- 4 focusing lens
- 5 pinhole
- 6 detector array

Figure B.2 — Measurement of the effective back or front focal length of a microlens array